

Zwischenrohr ZA 01/Q AF2
Intermediate tube ZA 01/Q AF2
nr./no. 515528


Wärmefalle PS 01/K AF1
Thermal Insulating tube PS 01/K AF1
nr./no. 513522

Axialluftdüse PS 01/A AF1
Air purge PS 01/A AF1
nr./no. 560951

PK Pyrometer

Befestigungswinkel Set PS 11/U
Set of mounting brackets PS 11/U
nr./no. 561537

Spülluftbedarf:
1 bis 10 ltr/min.
je nach erforderlicher Freiblaswirkung
Purging air requirements:
1 to 10 litres/min.
depending on blowing effect

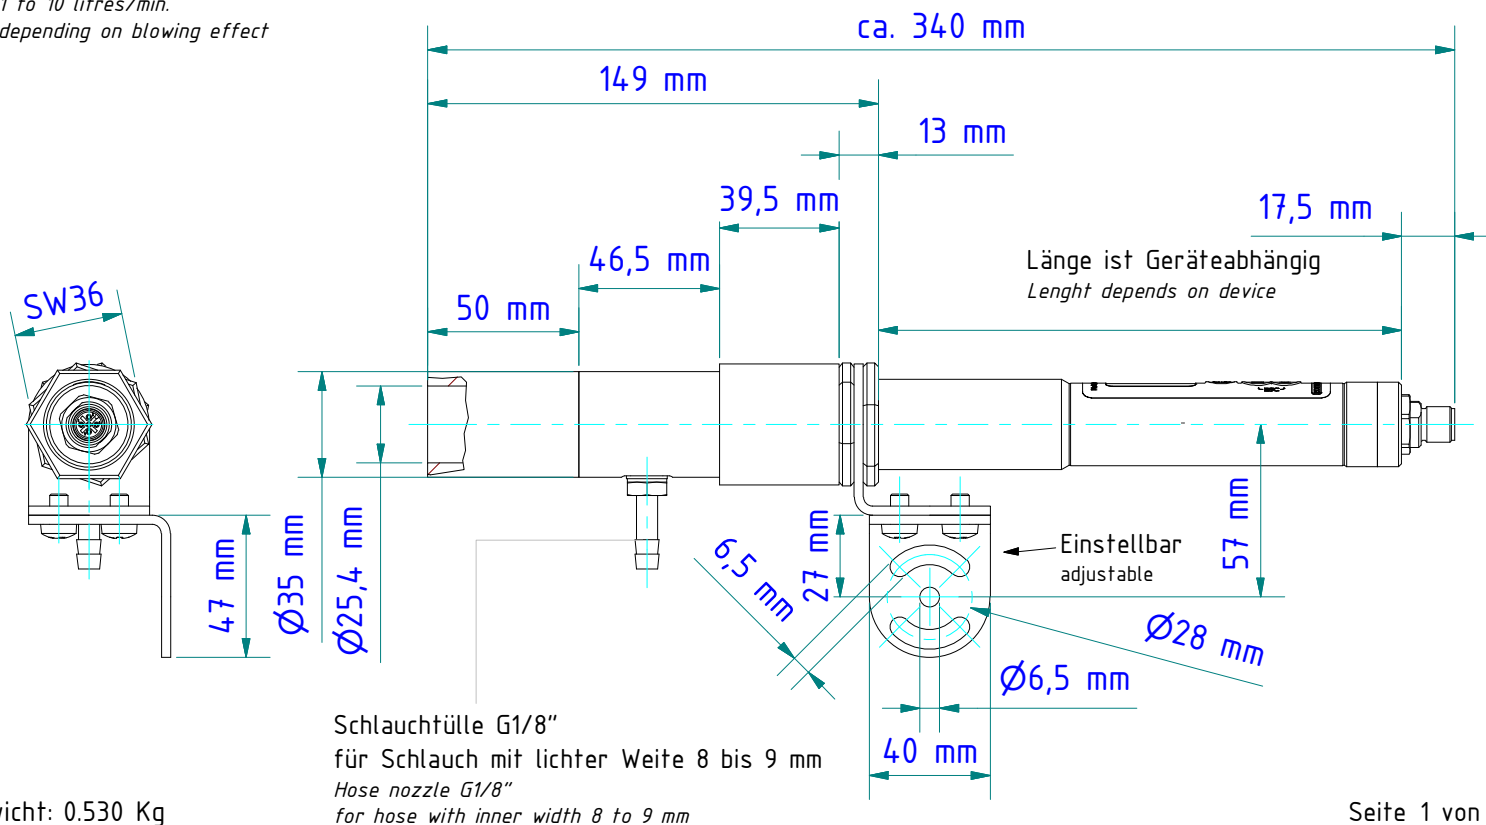

Seite 1 von 1
Page 1 of 1



- Headquarters
- Sales and Service Center
- Sales abroad



Keller HCW GmbH
Infrared Temperature Solutions (ITS)
Carl-Keller-Straße 2-10
49479 Ibbenbüren-Laggenbeck
Germany

www.keller.de/its
Tel. +49 (0) 5451 850
Fax +49 (0) 5451 85412
its@keller.de

Distributor



INOR Transmitter Oy
Unikkotie 13
FI-01300 Vantaa
Puhelin +358 10 4217900
Faksi +358 10 4217901
myynti@inor.fi