

★ Bei Verwendung mit einer Teleoptik (PA 20.06)
muss 1 Zwischenrohr ergänzt werden!
When using with a telephoto lens (PA 20.06),
1 intermediate tube must be added!

Kugelflansch PB 08/I AF1
Ball flange PB 08/I AF1
nr./no. 508167

Anbauflansch PZ 20/F
Flange PZ 20/F
nr./no. 561172

Axialluftdüse PZ 20/A AF1
Air purge PZ 20/A AF1
nr./no. 561176



Kühlarmatur geschlossen PA 20/M AF1
Cooling jacket closed PA 20/M AF1
nr./no. 1027765

Staubblende PZ 10/S
Dust stop PZ 10/S
nr./no. 561256

Zwischenrohr PZ 20/C
Intermediate tube PZ 20/C
nr./no. 561174

Saphir-Scheibenscharnier PZ 15/I AF2
Sapphire window with hinge PZ 15/I AF2
nr./no. 1066875

Pyrometer

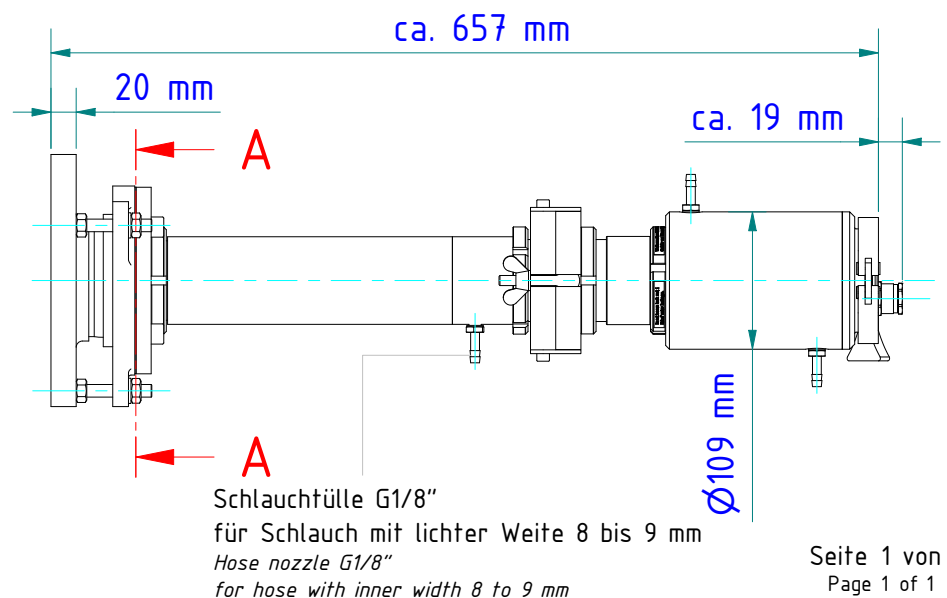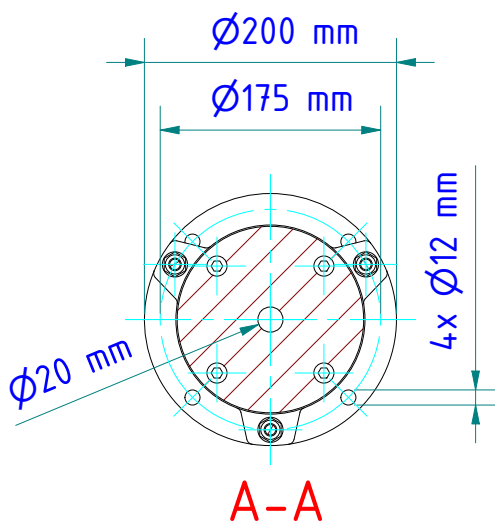

Gewicht: 10.170 Kg
Weight: 10.170 Kg

Seite 1 von 1
Page 1 of 1



- Headquarters
- Sales and Service Center
- Sales abroad



Keller HCW GmbH
Infrared Temperature Solutions (ITS)
Carl-Keller-Straße 2-10
49479 Ibbenbüren-Laggenbeck
Germany

www.keller.de/its
Tel. +49 (0) 5451 850
Fax +49 (0) 5451 85412
its@keller.de

Distributor



INOR Transmitter Oy
Unikkotie 13
FI-01300 Vantaa
Puhelin +358 10 4217900
Faksi +358 10 4217901
myynti@inor.fi