



nr./no.: 119158

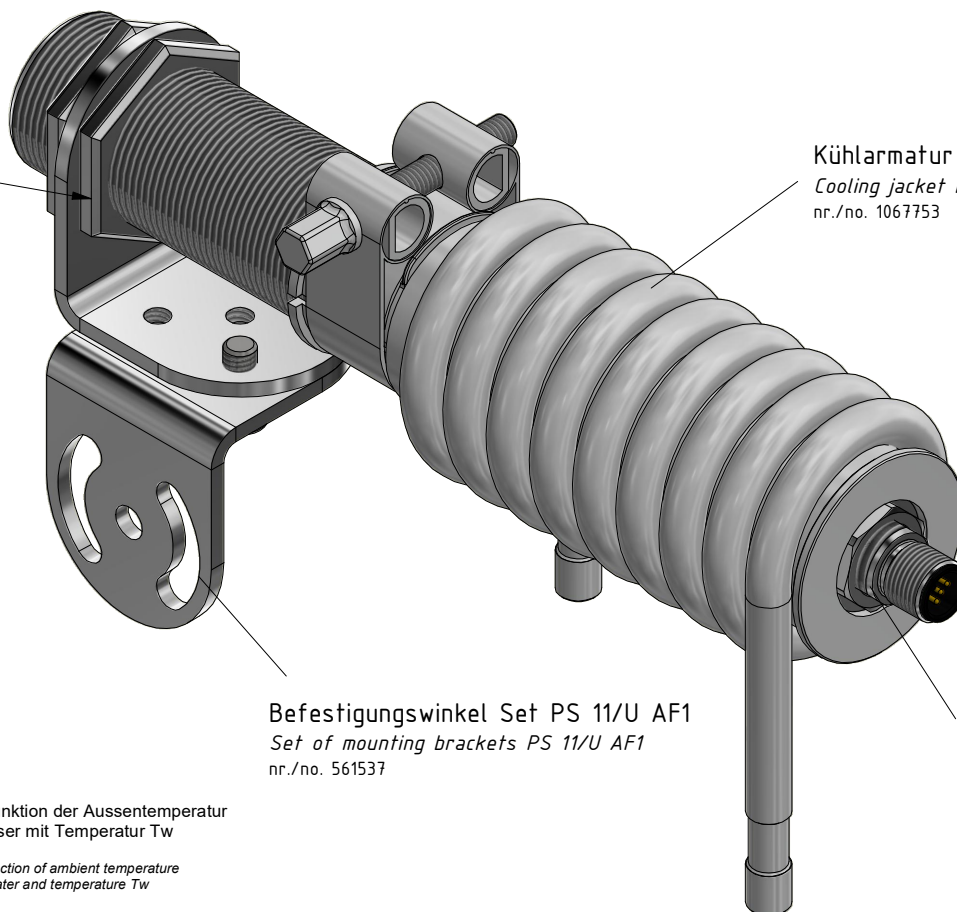

PK Pyrometer

- x— $T_w = 10^\circ\text{C}$
- Δ— $T_w = 20^\circ\text{C}$
- ◇— $T_w = 30^\circ\text{C}$
- $T_w = 40^\circ\text{C}$

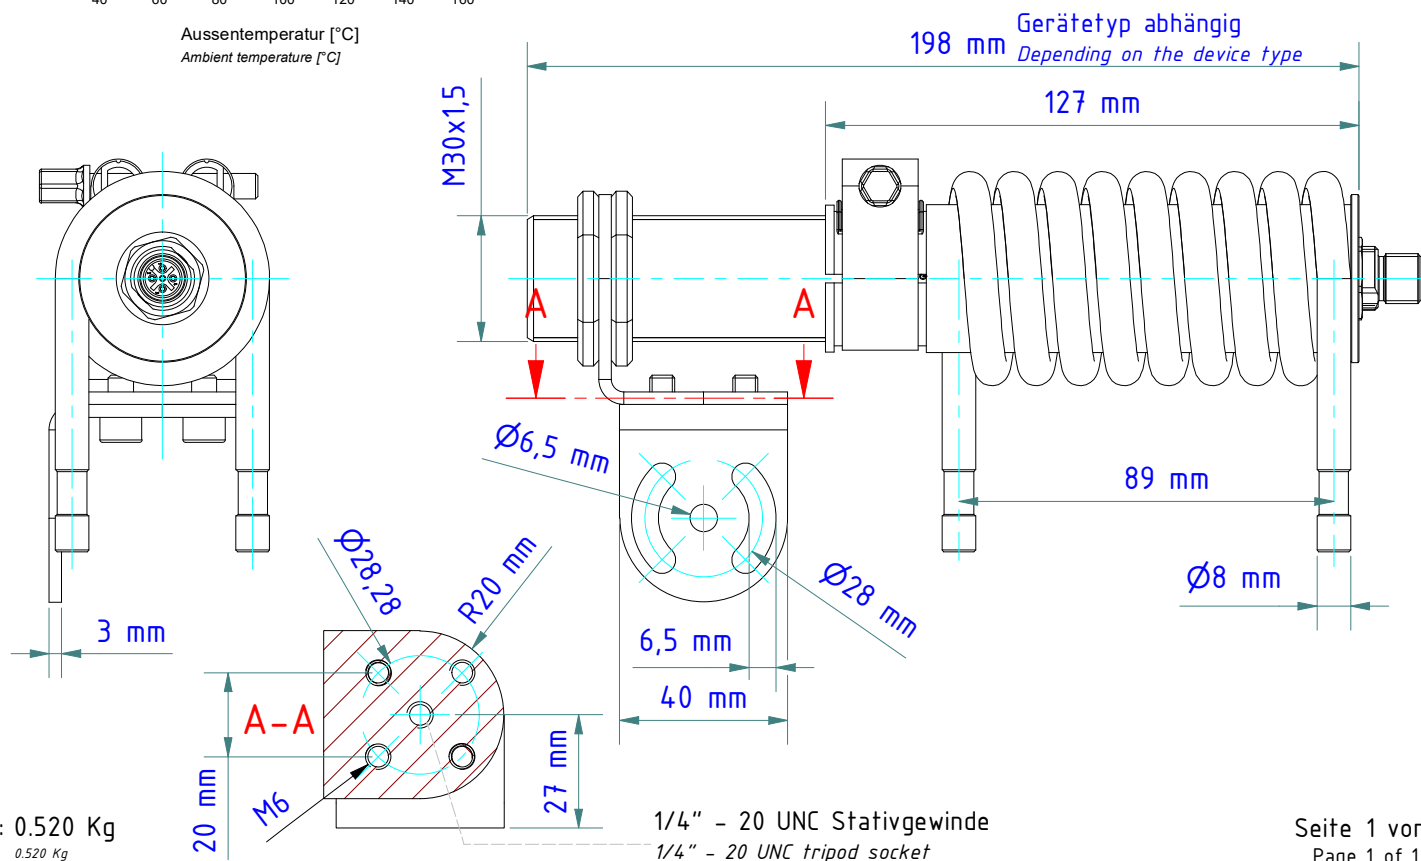

Seite 1 von 1
Page 1 of 1



- Headquarters
- Sales and Service Center
- Sales abroad



Keller HCW GmbH
Infrared Temperature Solutions (ITS)
Carl-Keller-Straße 2-10
49479 Ibbenbüren-Laggenbeck
Germany

www.keller.de/its
Tel. +49 (0) 5451 850
Fax +49 (0) 5451 85412
its@keller.de

Distributor



INOR Transmitter Oy
Unikkotie 13
FI-01300 Vantaa
Puhelin +358 10 4217900
Faksi +358 10 4217901
myynti@inor.fi